

TEST REPORT

Report No.: BCTC2311550268-1R

Applicant: Vincent Medical Excel Limited


Product Name: Red Light Tower



Product Type: RLC - VM


Tested Date: 2023-11-17 to 2024-01-30

Issued Date: 2024-03-05

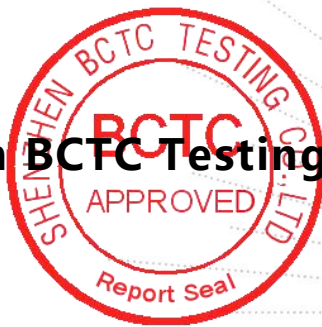Shenzhen BCTC Testing Co., Ltd.



Product Name	Red Light Tower
Product Type	RLC - VM
Applicant	Vincent Medical Excel Limited
Address	Units 1604-07A, 16/F., Two Harbourfront, 22 Tak Fung Street, Hung Hom, Kowloon, Hong Kong
Manufacturer	Vincent Medical(Dongguan)Technology Company Limited
Address	RM 101 And 201, Block 10, 1st Taoyuan Road, Songshan Lake Zone, Dongguan 523808, Guangdong P.R. China
Trademark	Clearlight
Sample Received Date	2023-11-17
Test Type	Entrustment Test
Test Method	Please refer to the following page(s).
Test Requested	<ol style="list-style-type: none"> As specified by client, to screen Lead(Pb), Cadmium(Cd), Mercury(Hg), Chromium(Cr) and Bromine(Br) in the submitted sample(s) by XRF. As specified by client, when screening results exceed the XRF screening limit in IEC 62321-3-1:2013, further use of chemical methods are required to test the Lead(Pb), Cadmium(Cd), Mercury(Hg), Hexavalent Chromium(Cr(VI)), Polybrominated Biphenyls(PBBs), Polybrominated Diphenyl Ethers(PBDEs) in the submitted sample(s). As specified by client, to test the Diisobutyl phthalate(DIBP), Dibutyl phthalate(DBP), Butyl benzyl phthalate(BBP), Bis(2-ethylhexyl) phthalate(DEHP) in the submitted sample(s).
Test Standard	RoHS Directive 2011/65/EU and amendment Commission Delegated Directive (EU) 2015/863
Test Result	The samples were tested according to the entrusted requirements and test standard, and the test items of the test samples were qualified.
Prepared by:	<div style="display: flex; justify-content: space-between;"> <div style="text-align: center;">  _____ Bear </div> <div style="text-align: center;">  _____ Saher Chen </div> </div>

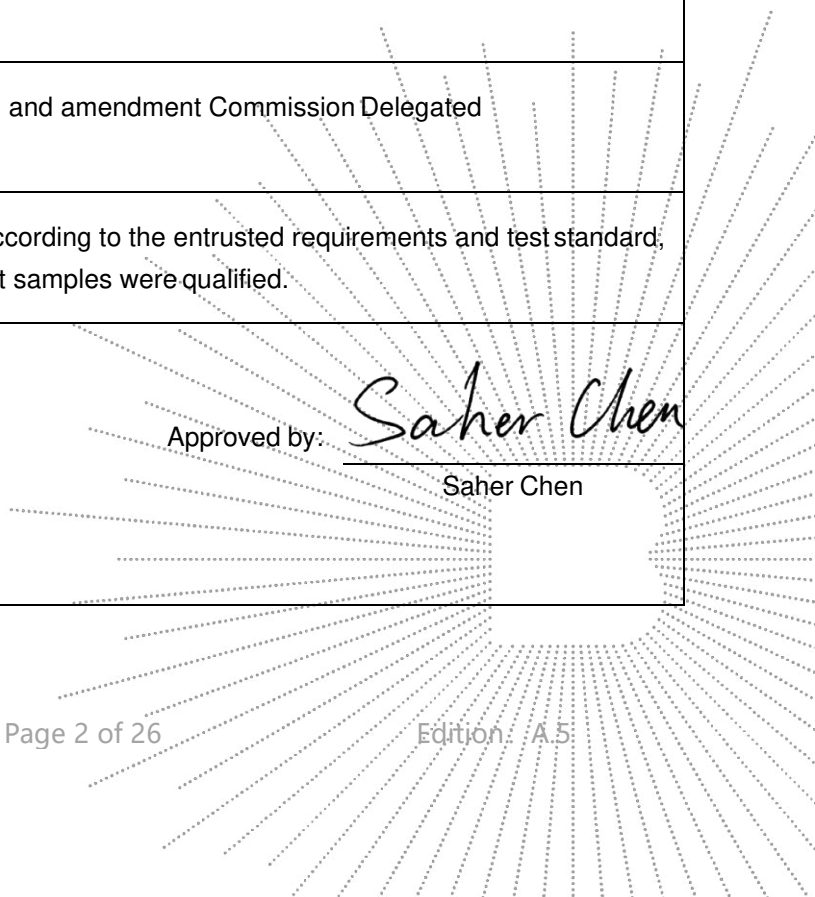


Test Method:
A. Screening test by XRF spectroscopy

XRF screening limits in mg/kg for regulated elements according to IEC 62321-3-1:2013.

Element	Screening limits of IEC 62321-3-1:2013 Unit (mg/kg)		MDL	
	Polymers and metals	Composite material	Polymers	Other material
Pb	$BL \leq (700 - 3\sigma) < X < (1300 + 3\sigma) \leq OL$	$BL \leq (500 - 3\sigma) < X < (1500 + 3\sigma) \leq OL$	10 mg/kg	50 mg/kg
Cd	$BL \leq (70 - 3\sigma) < X < (130 + 3\sigma) \leq OL$	$LOD < X < (150 + 3\sigma) \leq OL$	10 mg/kg	50 mg/kg
Hg	$BL \leq (700 - 3\sigma) < X < (1300 + 3\sigma) \leq OL$	$BL \leq (500 - 3\sigma) < X < (1500 + 3\sigma) \leq OL$	10 mg/kg	50 mg/kg
Cr	$BL \leq (700 - 3\sigma) < X$	$BL \leq (500 - 3\sigma) < X$	10 mg/kg	50 mg/kg
Br	$BL \leq (300 - 3\sigma) < X$	$BL \leq (250 - 3\sigma) < X$	10 mg/kg	50 mg/kg


Note:

- BL = Under the XRF screening limit
- OL = Further chemical test will be conducted while result is above the screening limit
- X= The symbol "X" marks the region where further investigation is necessary
- 3σ= The reproducibility of analytical instruments
- LOD= Detection limit
- "-" = Not regulated.

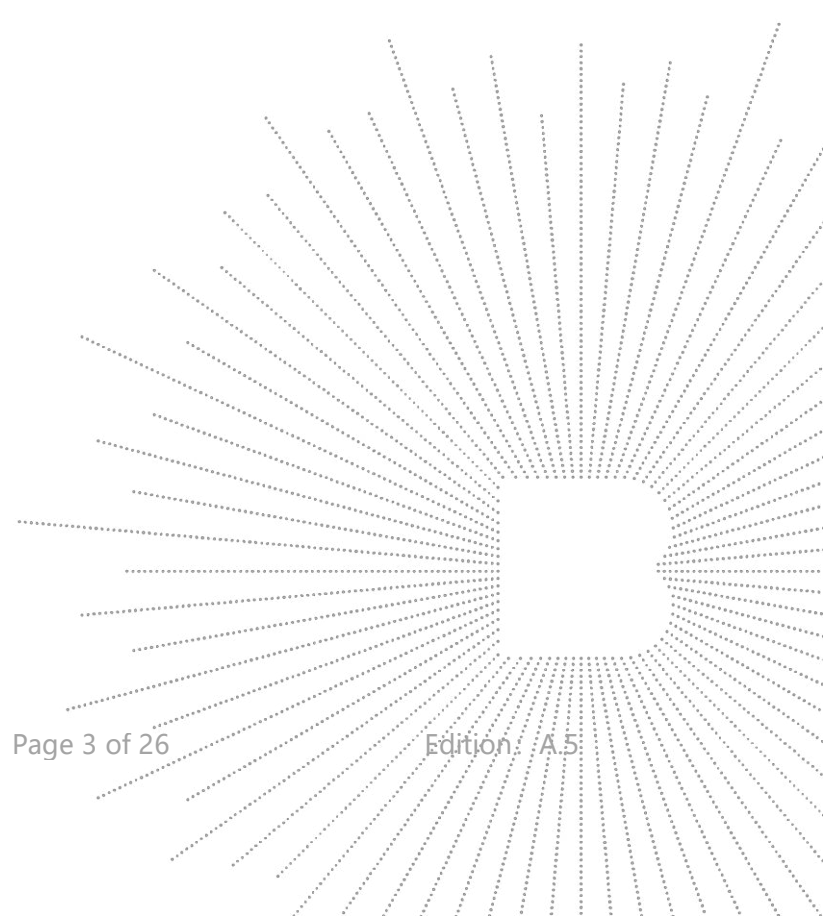 BCTC
 3C
 PPR
 Report


B. Chemical Test

Test Item(s)	Test Method	Measured Equipment(s)	MDL	Limit
Lead (Pb)	IEC 62321-5:2013 Ed.1.0	ICP-OES	2 mg/kg	1000 mg/kg
Cadmium (Cd)	IEC 62321-5:2013 Ed.1.0	ICP-OES	2 mg/kg	100 mg/kg
Mercury (Hg)	IEC 62321-4:2013+AMD1:2017	ICP-OES	2 mg/kg	1000 mg/kg
Hexavalent Chromium Cr(VI)	IEC 62321-7-1:2015 Ed.1.0	UV-VIS	--	1000 mg/kg
	IEC 62321-7-2:2017 Ed.1.0		8 mg/kg	1000 mg/kg
Polybrominated Biphenyls (PBBs)	IEC 62321-6:2015 Ed.1.0	HPLC-UV	5 mg/kg	1000 mg/kg
Polybrominated Diphenyl Ethers (PBDEs)	IEC 62321-6:2015 Ed.1.0	HPLC-UV	5 mg/kg	1000 mg/kg
Diisobutyl phthalate (DIBP)	IEC 62321-8:2017 Ed.1.0	GC-MS	50 mg/kg	1000 mg/kg
Dibutyl phthalate (DBP)	IEC 62321-8:2017 Ed.1.0	GC-MS	50 mg/kg	1000 mg/kg
Butyl benzyl phthalate (BBP)	IEC 62321-8:2017 Ed.1.0	GC-MS	50 mg/kg	1000 mg/kg
Bis(2-ethylhexyl) phthalate (DEHP)	IEC 62321-8:2017 Ed.1.0	GC-MS	50 mg/kg	1000 mg/kg

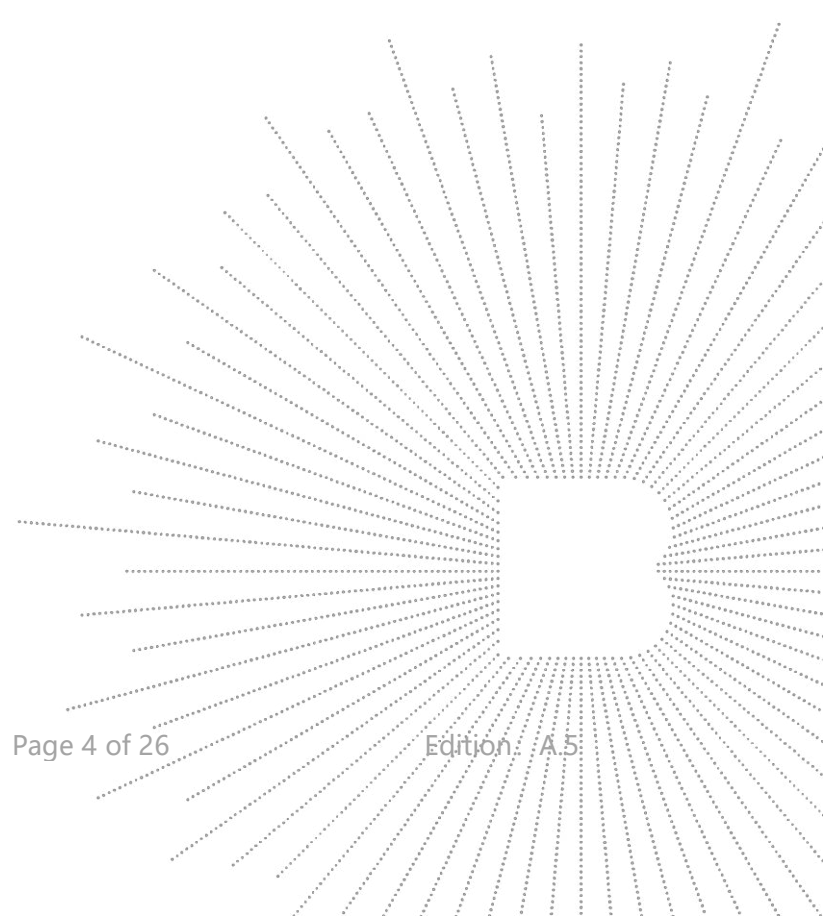

TE
 TC
 OVE
 t See

Test Result(s):

Sample No.	Sample Description	Tested Items	XRF Screening Test Unit (mg/kg)	Chemical Test Unit (mg/kg)	Conclusion
1	Metal with black plating	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	806	Negative	
		Br(PBBs&PBDEs)	/	/	
2	Silver plastic	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	BL	/	
3	Transparent plastic	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	BL	/	
4	White light board	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	BL	/	
5	SMD LED	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	BL	/	
6	White plastic	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	BL	/	
7	Silver metal	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	/	/	

8	IC	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	BL	/	
9	Blue green patch	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	BL	/	
10	Yellow epoxy board	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	BL	/	
11	Green FPC	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	BL	/	
12	Silver metal	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	1241	Negative	
		Br(PBBs&PBDEs)	/	/	
13	Black outside wire jacket	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	BL	/	
14	Yellow green wire jacket	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	BL	/	
15	Blue wire jacket	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	BL	/	

CO.,LTD

16	Brown wire jacket	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	BL	/	
17	Silver metal contact sheet	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	/	/	
18	Black plastic	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	33171	N.D.	
19	Silver metal	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	/	/	
20	Blue plastic	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	BL	/	
21	Black rubber	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	BL	/	
22	Silver metal	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	/	/	
23	White plastic	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	BL	/	


24	Black plastic	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	BL	/	
25	Silver metal	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	/	/	
26	Silver metal	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	/	/	
27	Silver metal	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	/	/	
28	Black wire jacket	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	BL	/	
29	Red wire jacket	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	BL	/	
30	White plastic	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	BL	/	
31	Black plastic	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	BL	/	



32	Black plastic	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	60256	N.D.	
33	Blue PCB	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	BL	/	
34	Tin solder	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	/	/	
35	Black wire jacket	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	BL	/	
36	Red wire jacket	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	BL	/	
37	Black plastic	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	BL	/	
38	Silver metal	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	/	/	
39	White plastic	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	67566	N.D.	


40	Copper metal	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	/	/	
41	Black outside wire jacket	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	BL	/	
42	Black PCB	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	BL	/	
43	Green PCB	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	15895	N.D.	
44	Tin solder	Pb	BL	/	PASS
		Cd	BL	/	
		Hg	BL	/	
		Cr(Cr(VI))	BL	/	
		Br(PBBs&PBDEs)	/	/	

TE
TC
OV
t See

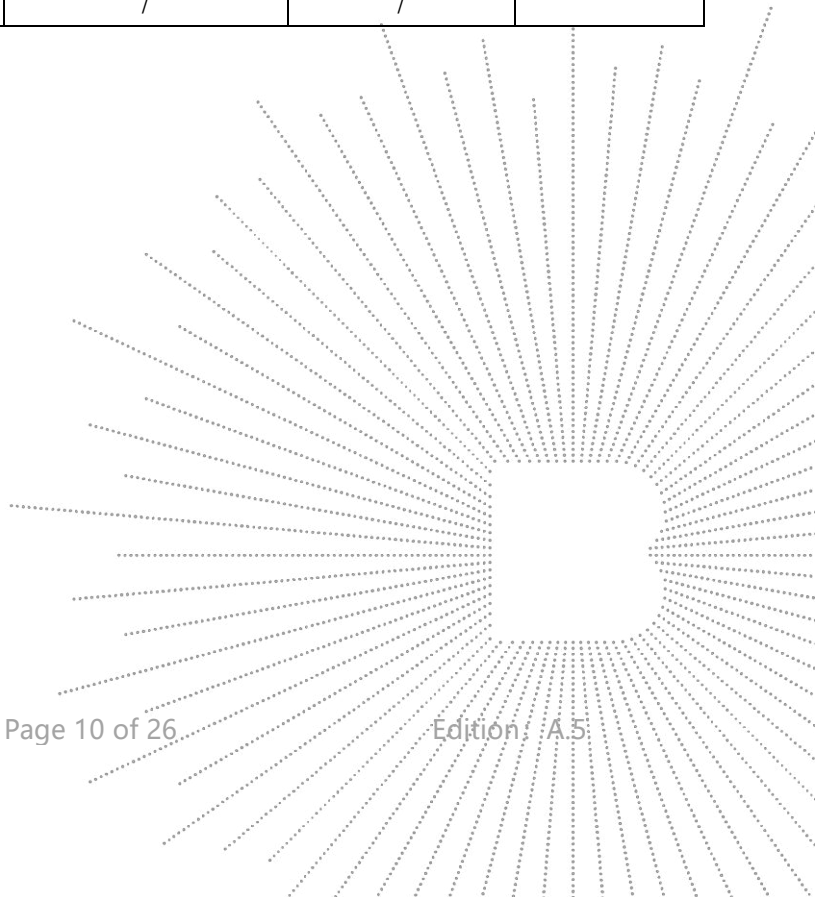

Tested Item(s)	Results Unit (mg/kg)							
	2	3	5+8+10	9	11	13	14	15
Diisobutyl phthalate(DIBP) CAS No.:84-69-5	N.D.	N.D.	N.D.	N.D.	N.D.	N.D.	N.D.	N.D.
Dibutyl phthalate(DBP) CAS No.:84-74-2	N.D.	N.D.	N.D.	N.D.	N.D.	N.D.	N.D.	N.D.
Butyl benzyl phthalate(BBP) CAS No.:85-68-7	N.D.	N.D.	N.D.	N.D.	N.D.	N.D.	N.D.	N.D.
Bis(2-ethylhexyl) phthalate(DEHP) CAS No.:117-81-7	N.D.	N.D.	N.D.	N.D.	N.D.	94	N.D.	N.D.

Tested Item(s)	Results Unit (mg/kg)						
	16	18	20	21	23	24+30+32	28
Diisobutyl phthalate(DIBP) CAS No.:84-69-5	N.D.	N.D.	N.D.	N.D.	N.D.	N.D.	N.D.
Dibutyl phthalate(DBP) CAS No.:84-74-2	N.D.	N.D.	N.D.	N.D.	N.D.	N.D.	495
Butyl benzyl phthalate(BBP) CAS No.:85-68-7	N.D.	N.D.	N.D.	N.D.	N.D.	N.D.	N.D.
Bis(2-ethylhexyl) phthalate(DEHP) CAS No.:117-81-7	N.D.	N.D.	N.D.	N.D.	N.D.	N.D.	91

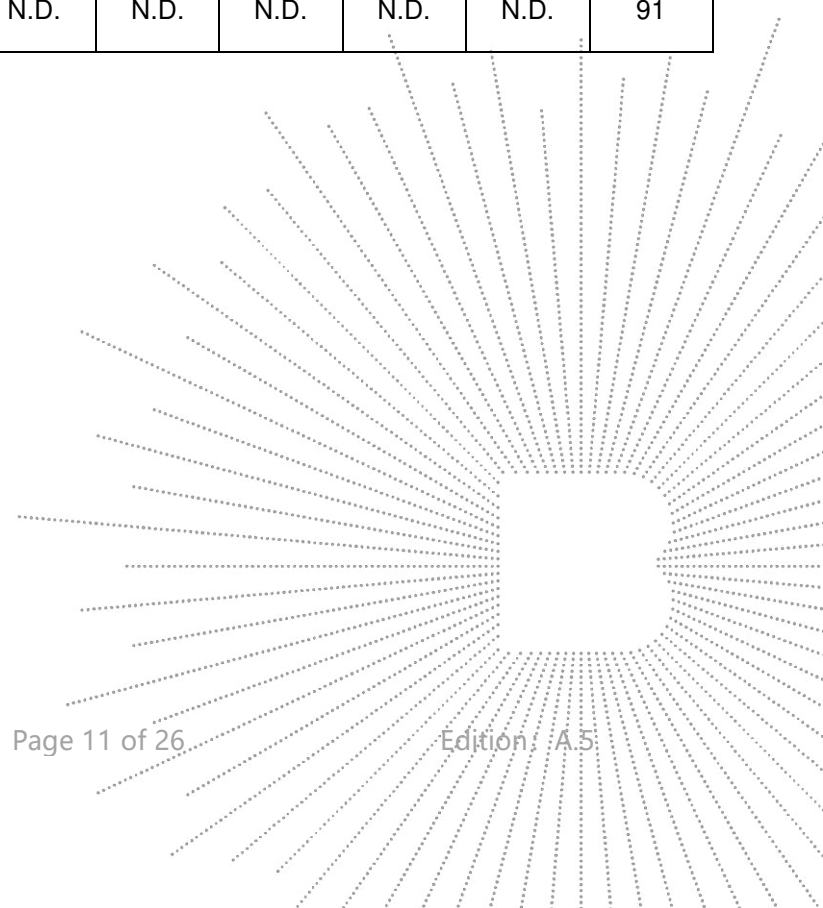

Tested Item(s)	Results							
	Unit (mg/kg)							
	29	31	33	35	36	37	39+42 +43	41
Diisobutyl phthalate(DIBP) CAS No.:84-69-5	N.D.	N.D.	N.D.	N.D.	N.D.	N.D.	N.D.	N.D.
Dibutyl phthalate(DBP) CAS No.:84-74-2	N.D.	N.D.	N.D.	180	141	N.D.	N.D.	N.D.
Butyl benzyl phthalate(BBP) CAS No.:85-68-7	N.D.	N.D.	N.D.	N.D.	N.D.	N.D.	N.D.	N.D.
Bis(2-ethylhexyl) phthalate(DEHP) CAS No.:117-81-7	N.D.	N.D.	N.D.	65	N.D.	N.D.	N.D.	N.D.

Note:

-MDL = Method Detection Limit

-N.D. = Not Detected (<MDL)

-mg/kg = ppm = parts per million

-" / " = Not conducted.

-Negative = Absence of Cr(VI), the detected Cr(VI) concentration in the boiling water extraction solution is less than 0.1µg/cm² with 50cm² sample surface area used.


-Positive = Presence of Cr(VI), the detected Cr(VI) concentration in the boiling water extraction solution is equal to or greater than 0.13µg/cm² with 50cm² sample surface area used.

Remark:

-The screening results are only used for reference.

-When conducting the test for PBBs&PBDEs, XRF was introduced to screen Br Exclusively; When conducting the test for Hexavalent Chromium, XRF was introduced to screen Chromium exclusively.


CO., LTD.

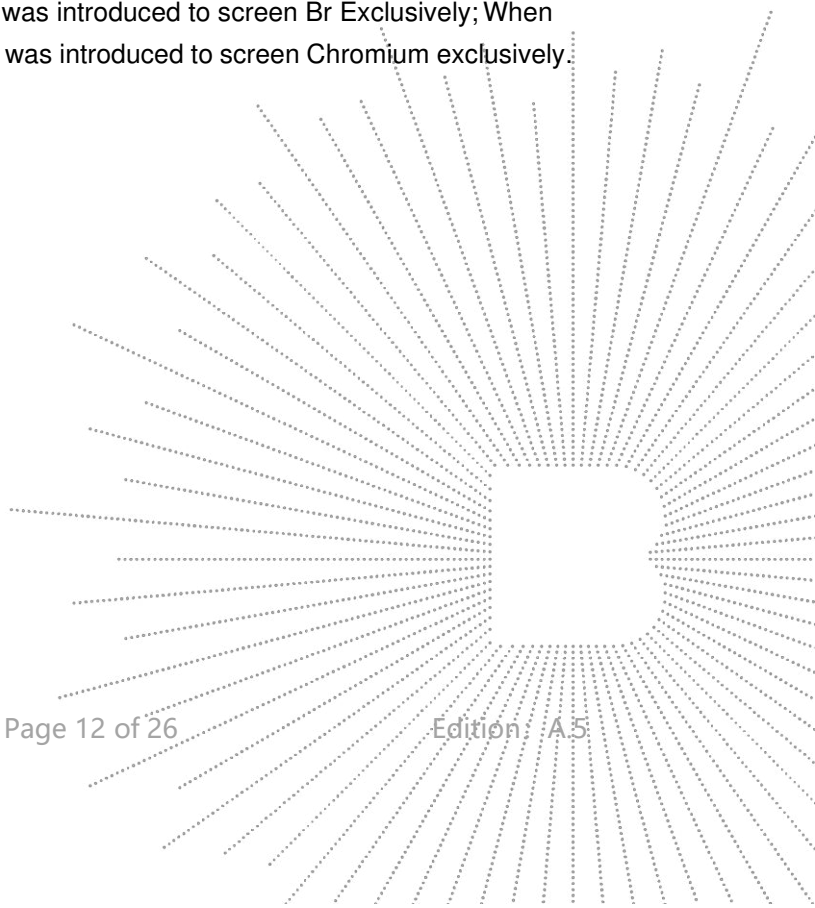


Test Process:

The sample(s) had been dissolved totally tested for Lead, Cadmium, Mercury.

◆ IEC 62321-5:2013 Ed.1.0

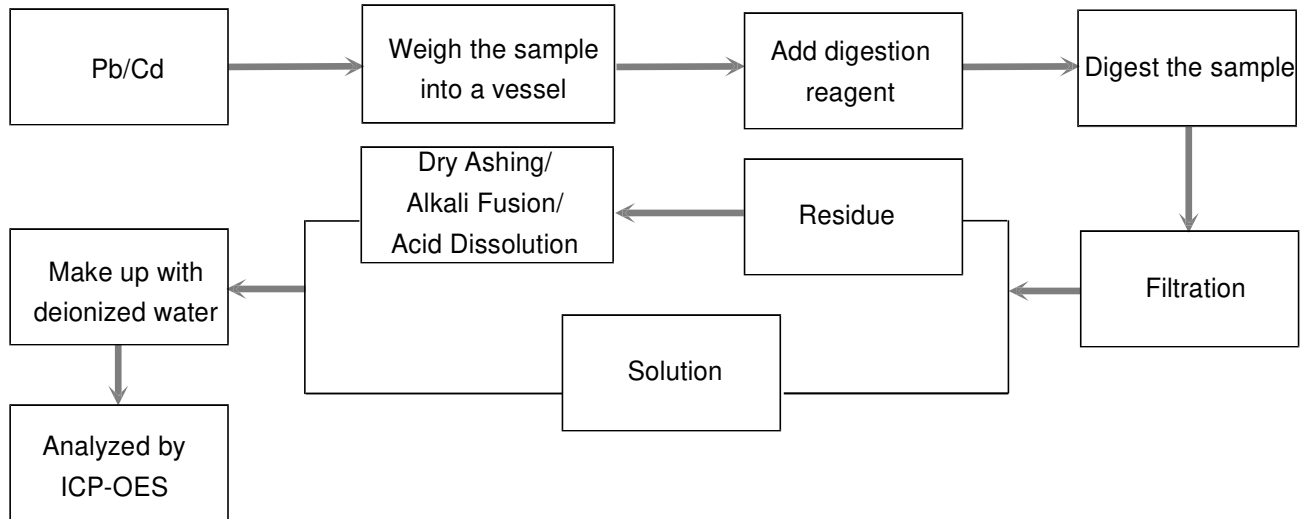


◆ IEC 62321-4:2013+AMD1:2017


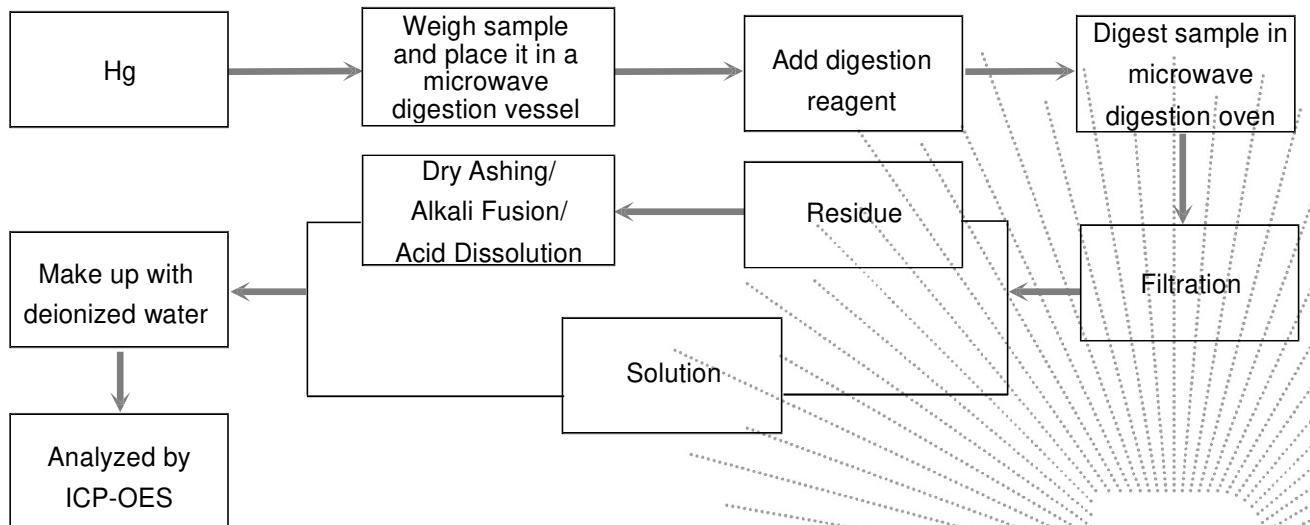


CHENZHEN


◆ IEC 62321-7-1:2015 Ed.1.0

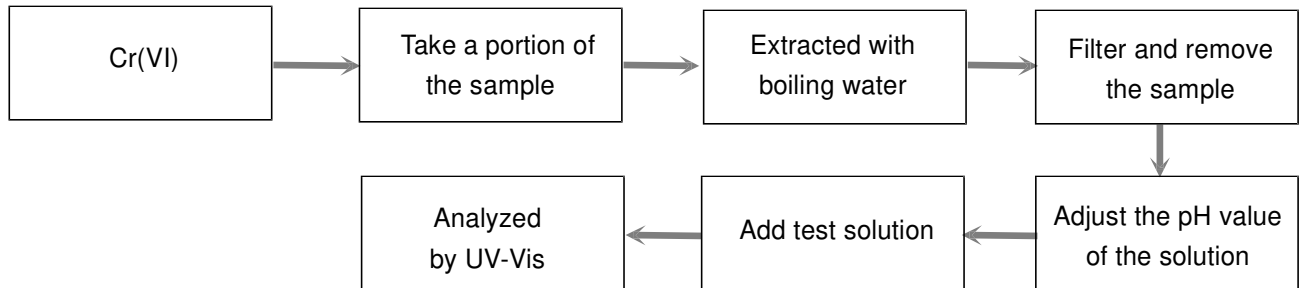


◆ IEC 62321-7-2:2017 Ed.1.0

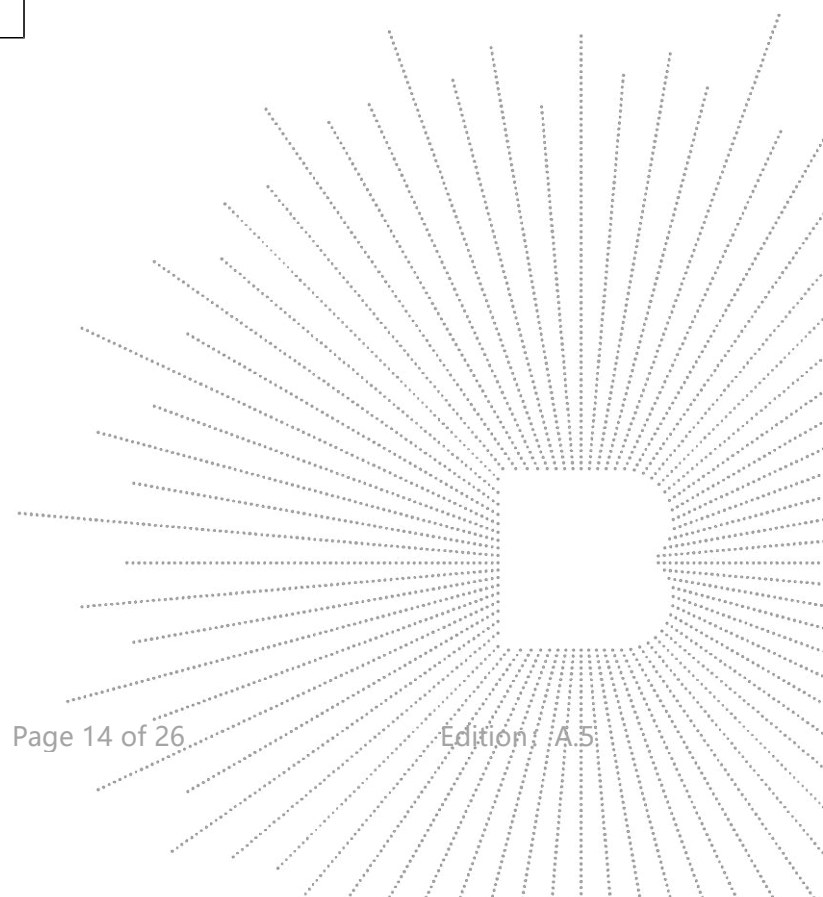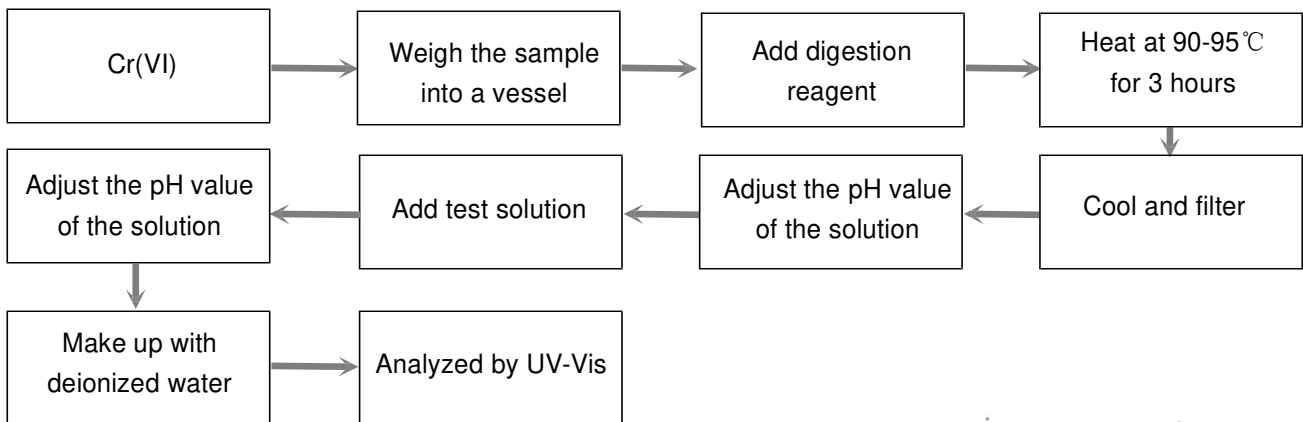


◆ IEC 62321-6:2015 Ed.1.0

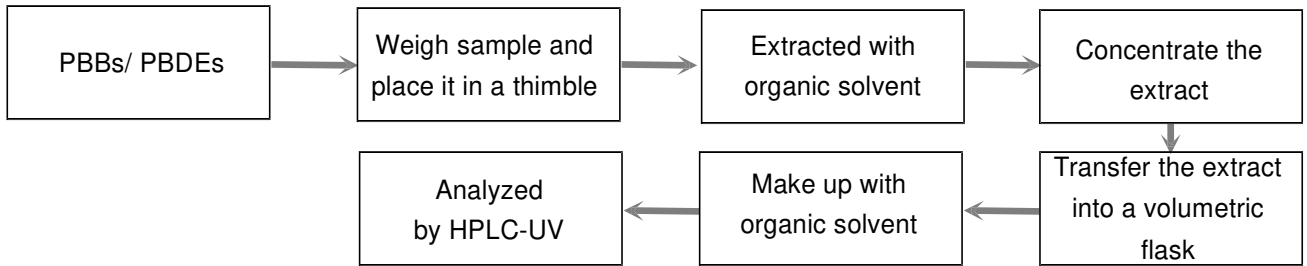

◆ IEC 62321-8:2017 Ed.1.0

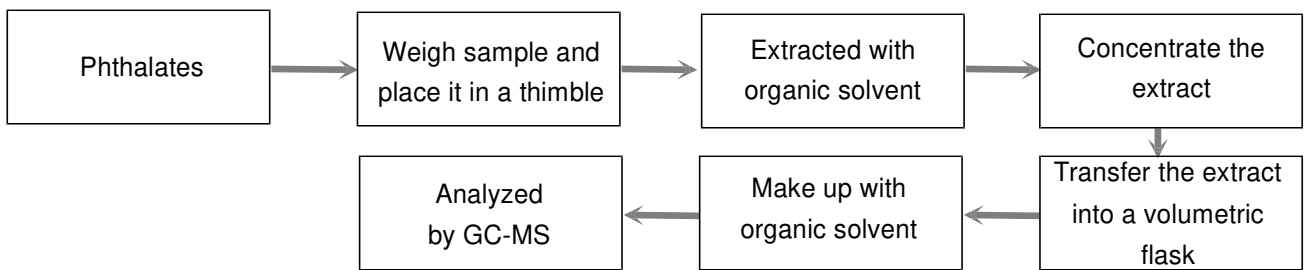

BCTC
3C
PPR
Report

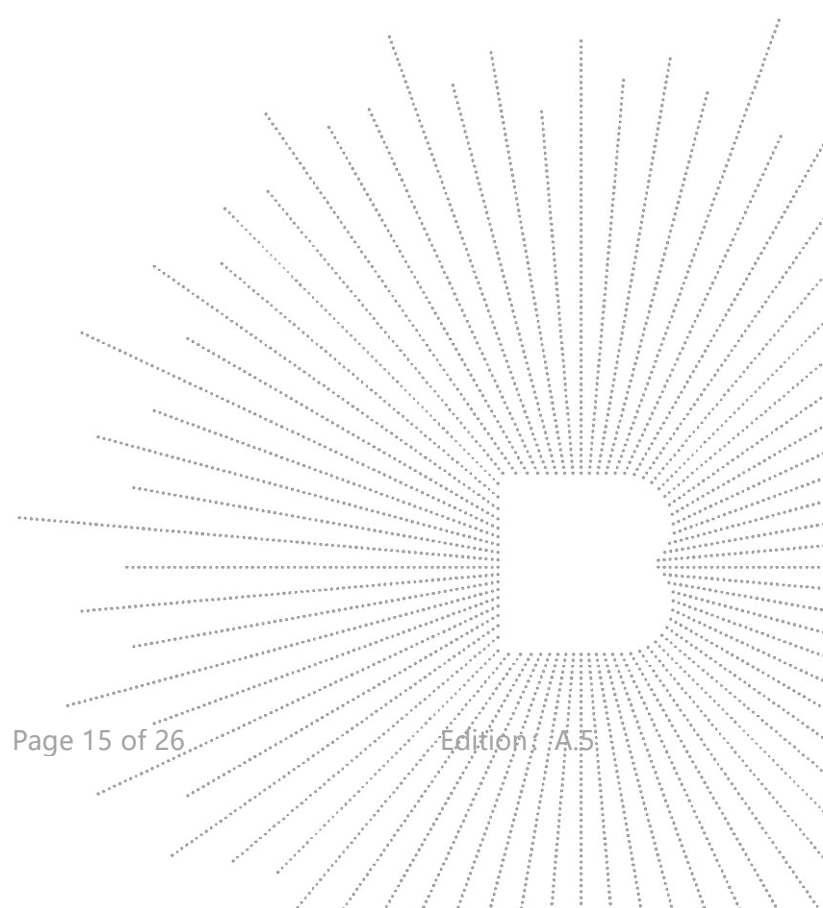

Photograph of Sample

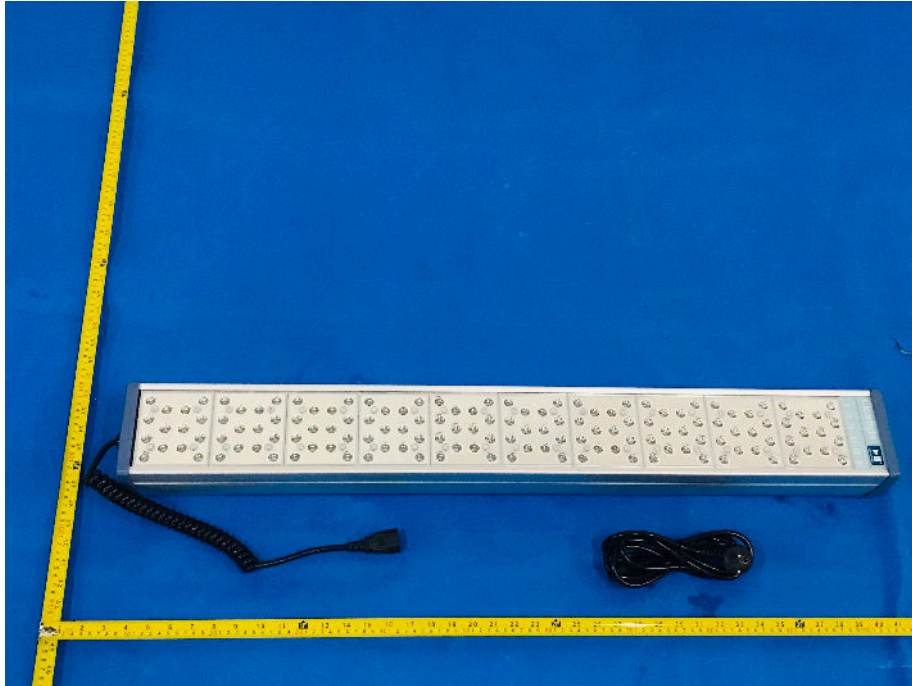


Fig.1


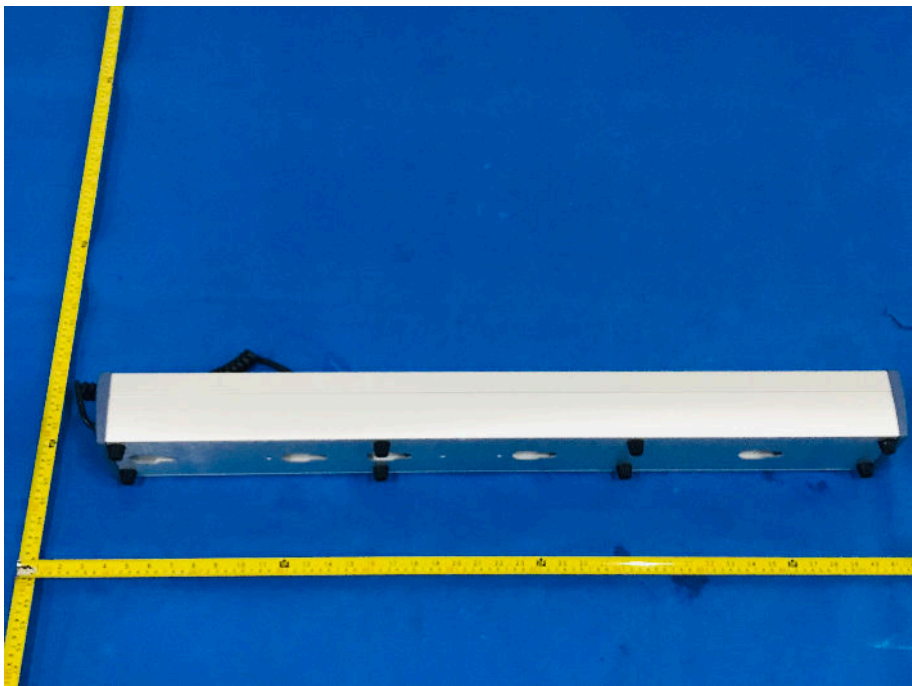


Fig.2

TEC
TC
OVB
t See

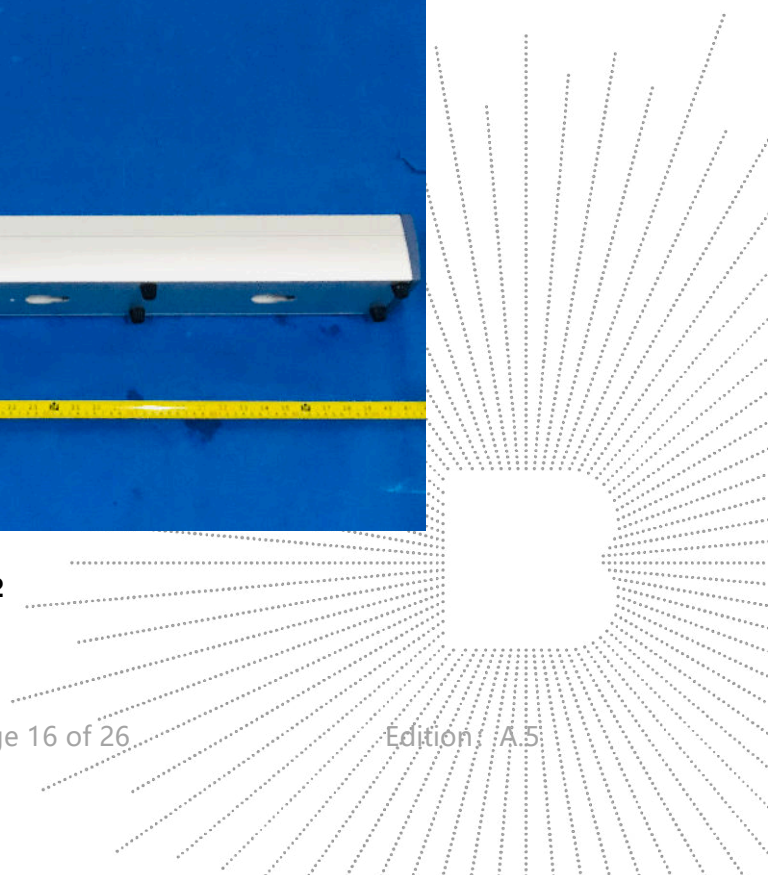

Photo(s) of the tested component(s)

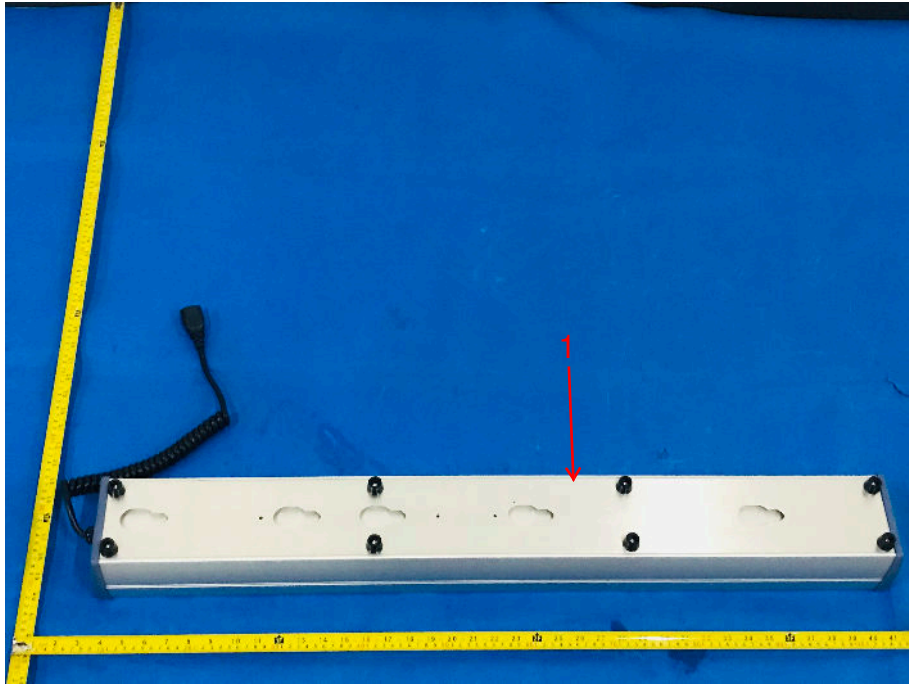


Fig.3

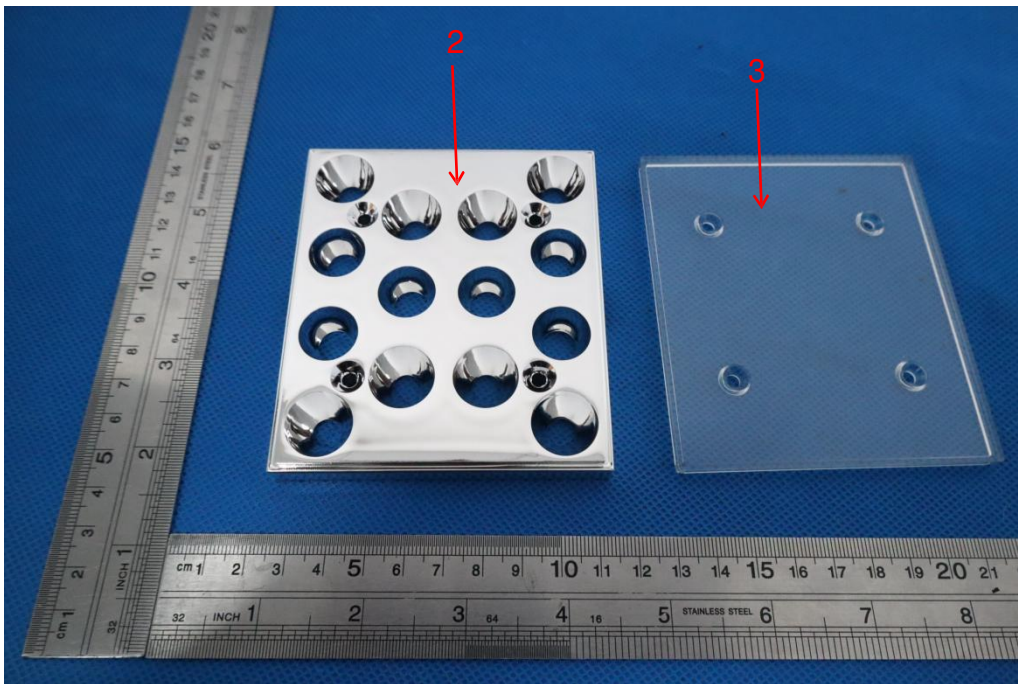
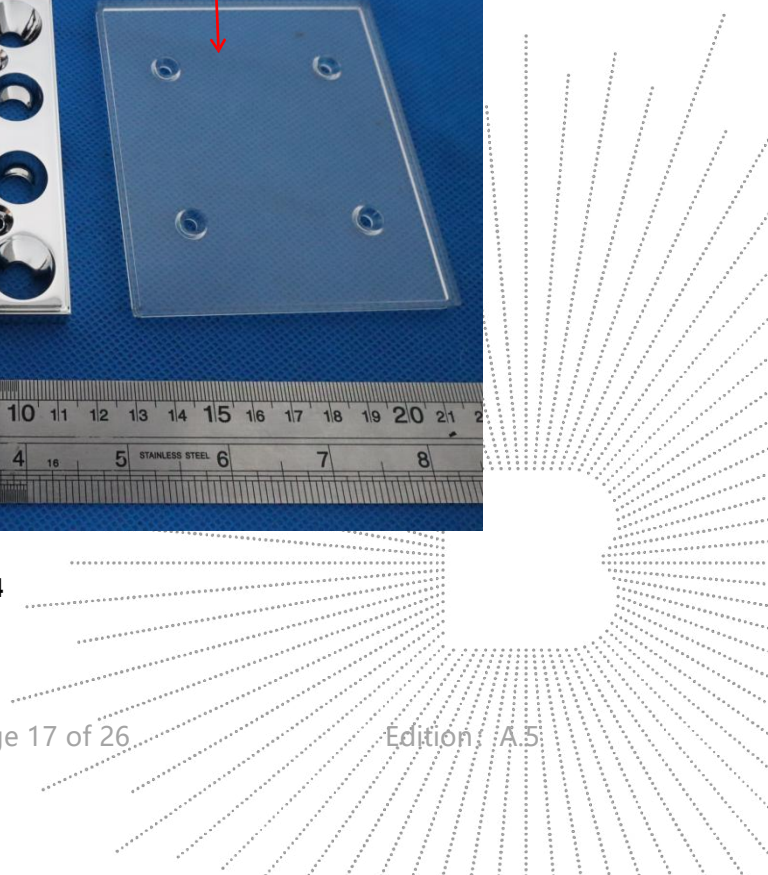


Fig.4



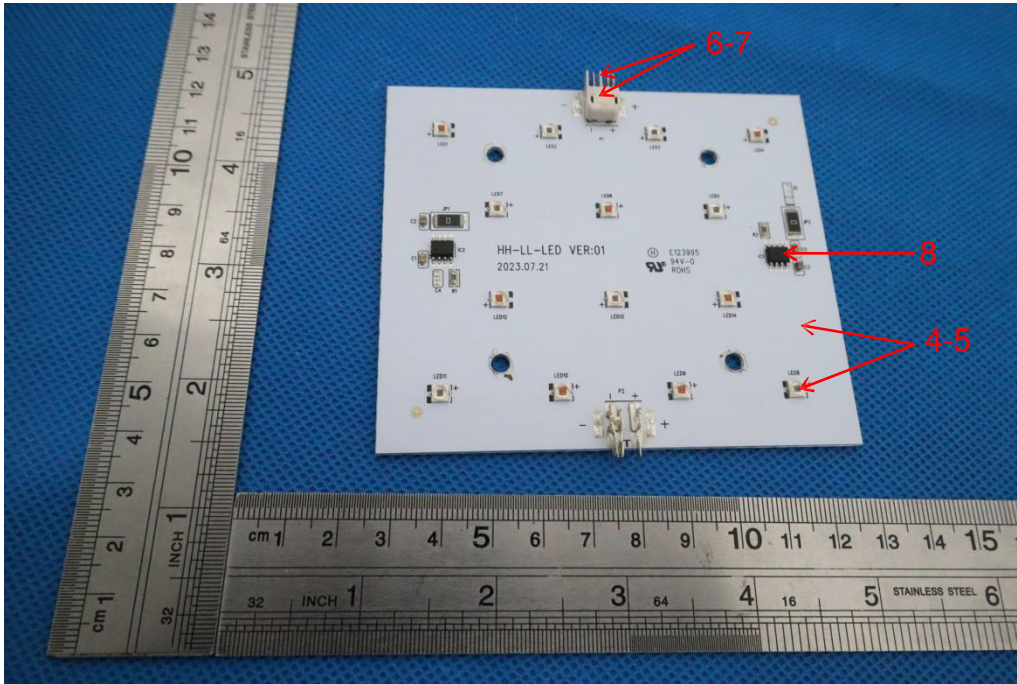


Fig.5

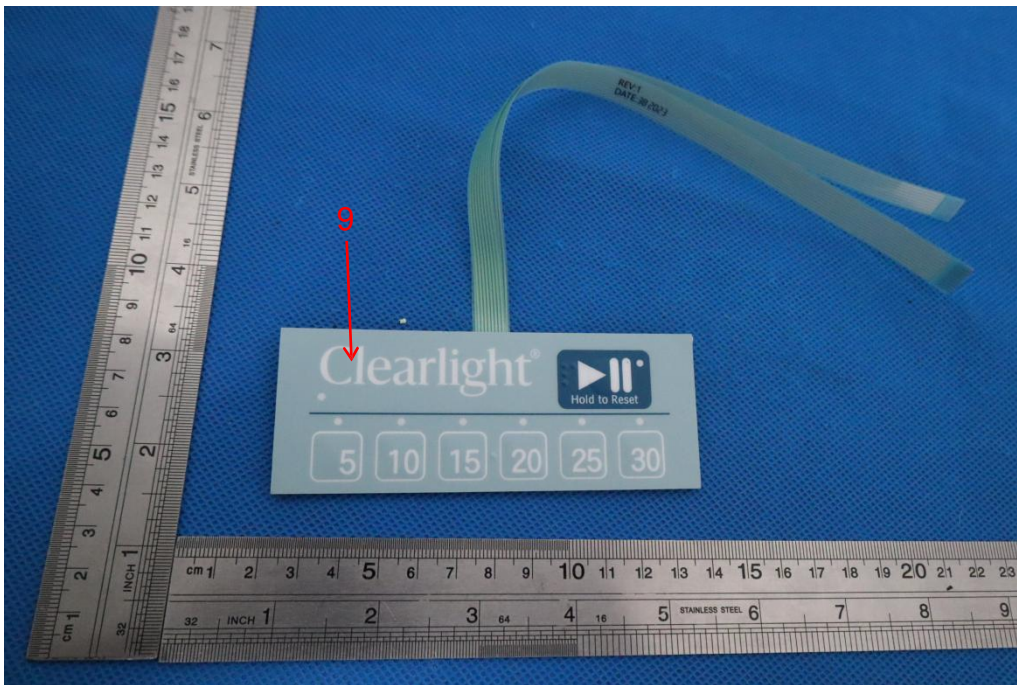


Fig.6

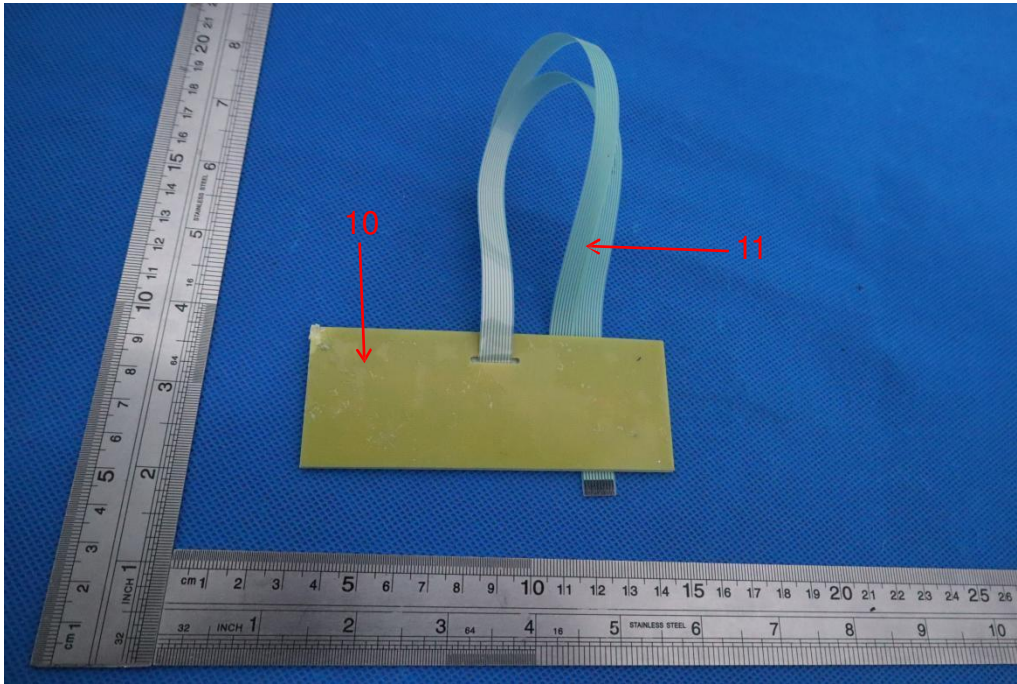


Fig.7

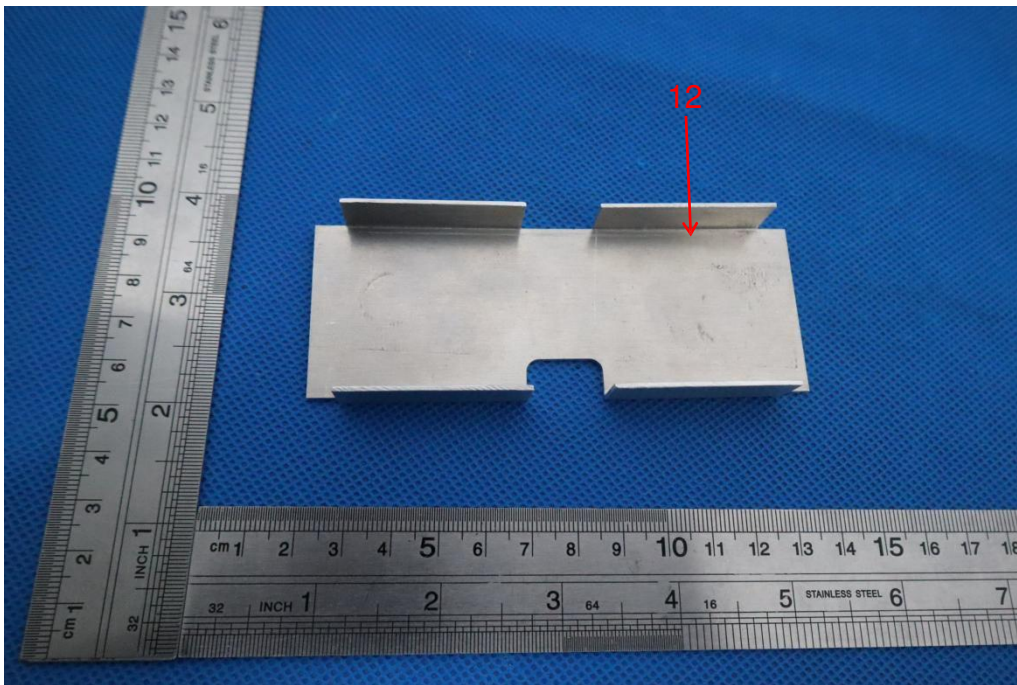
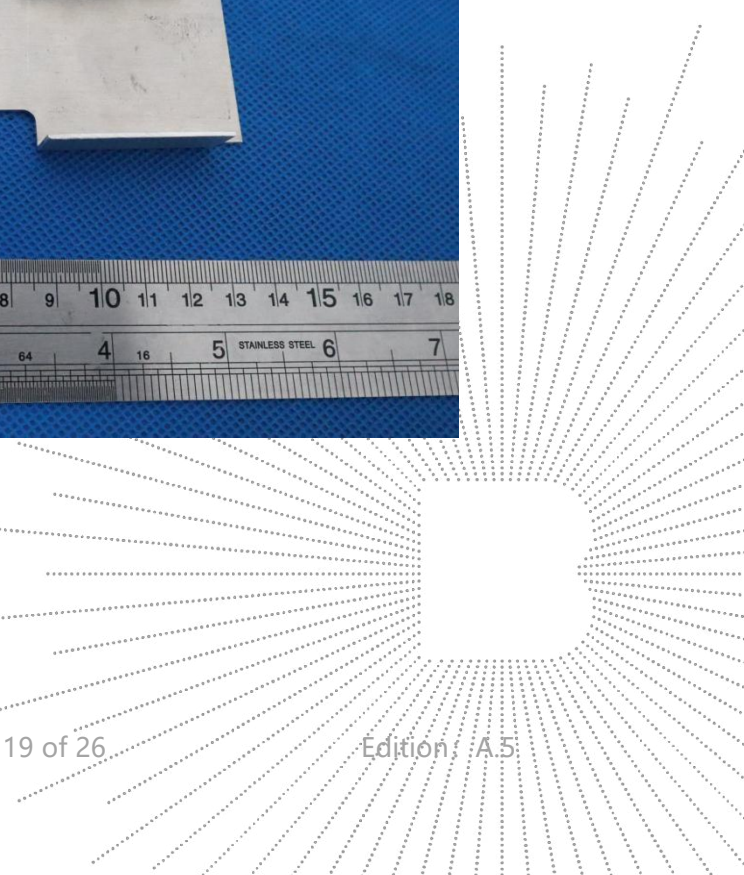


Fig.8



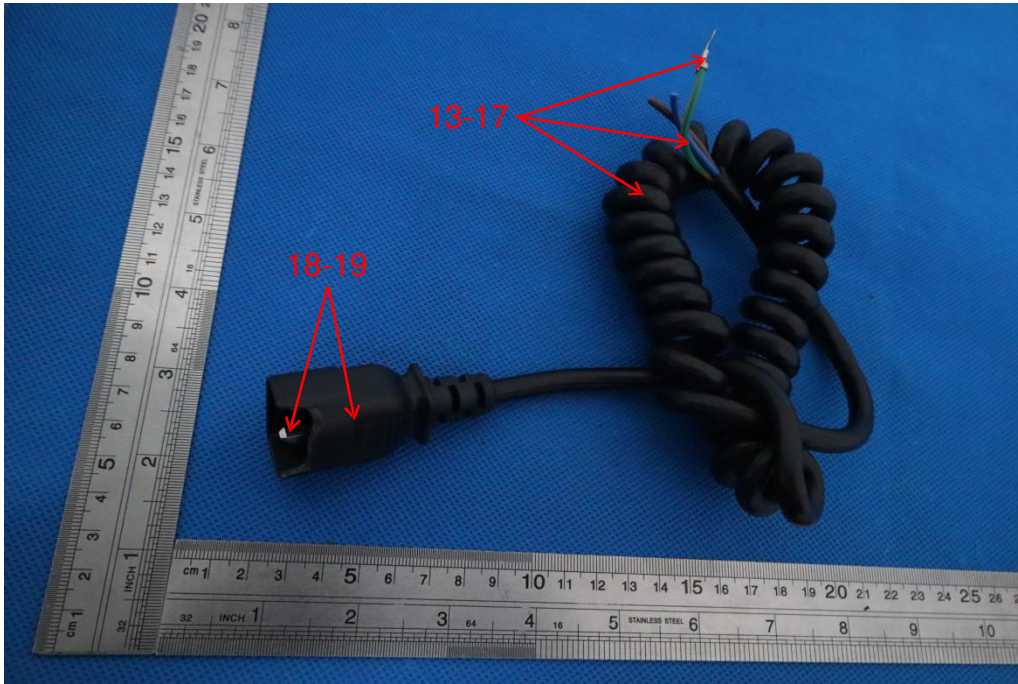


Fig.9

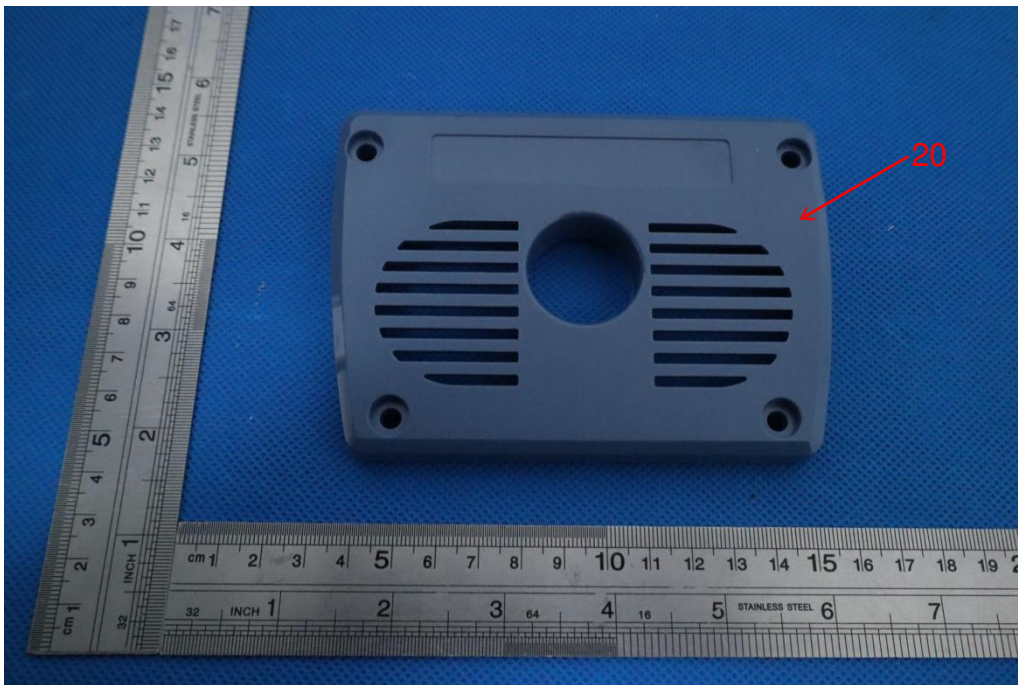


Fig.10

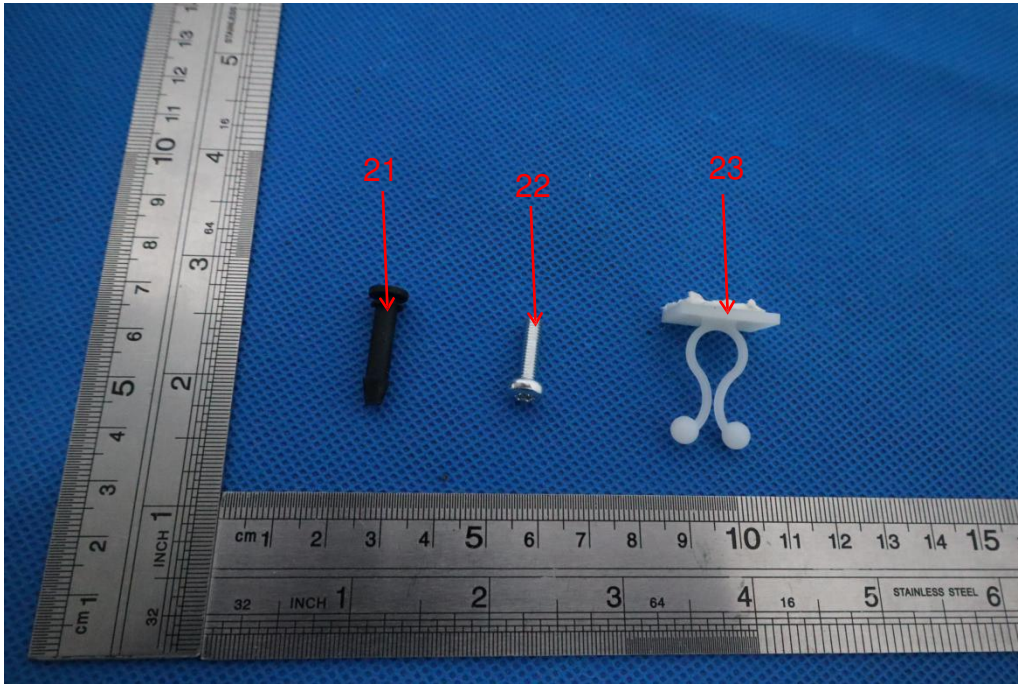


Fig.11

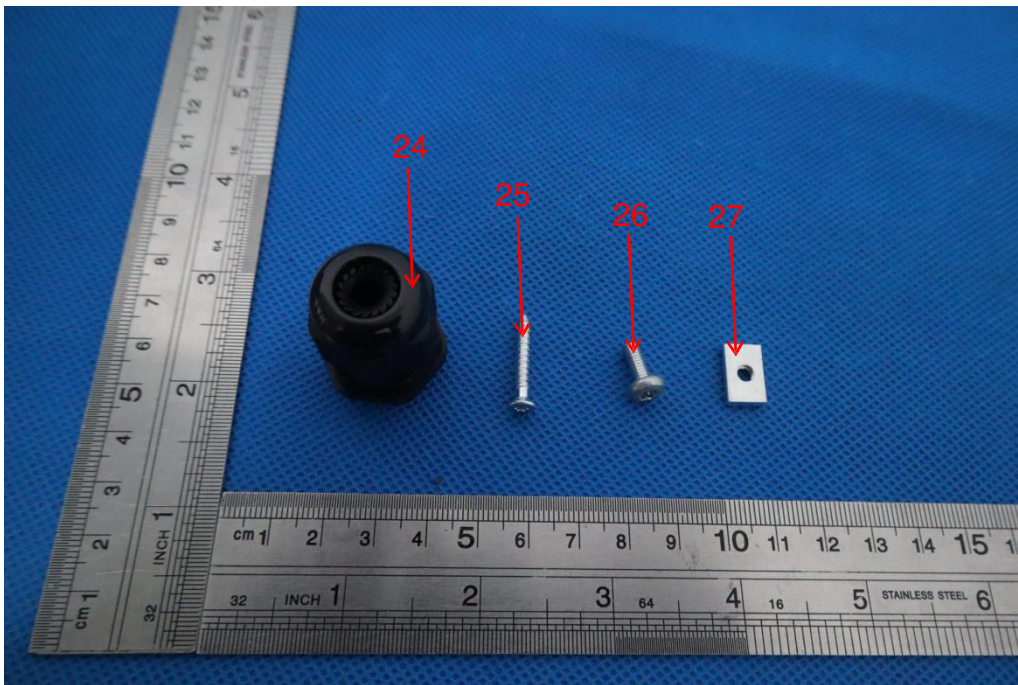
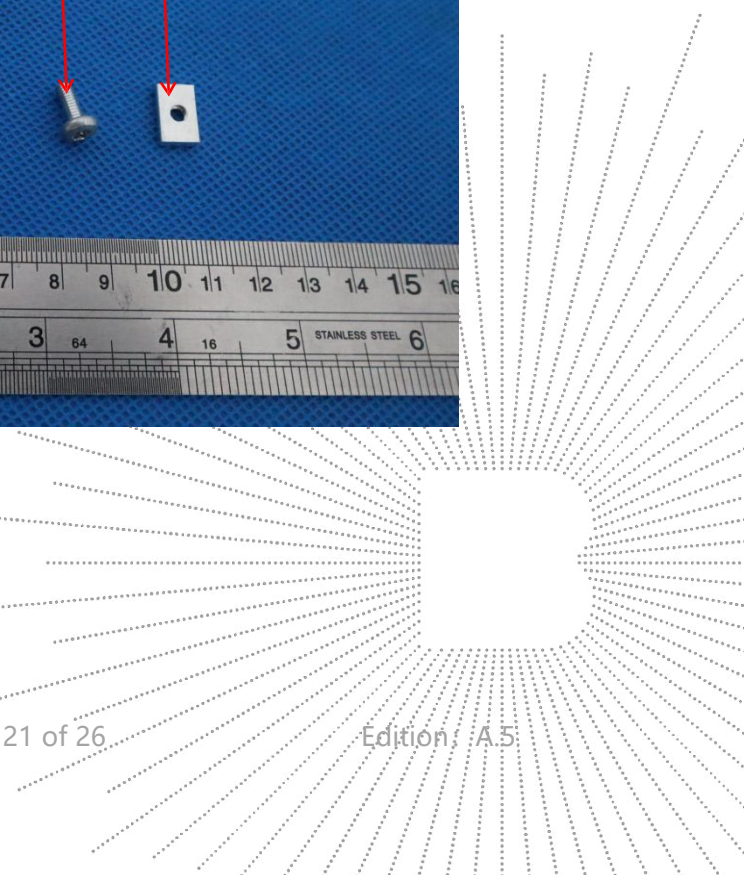


Fig.12

BCTC
B
AP
Re



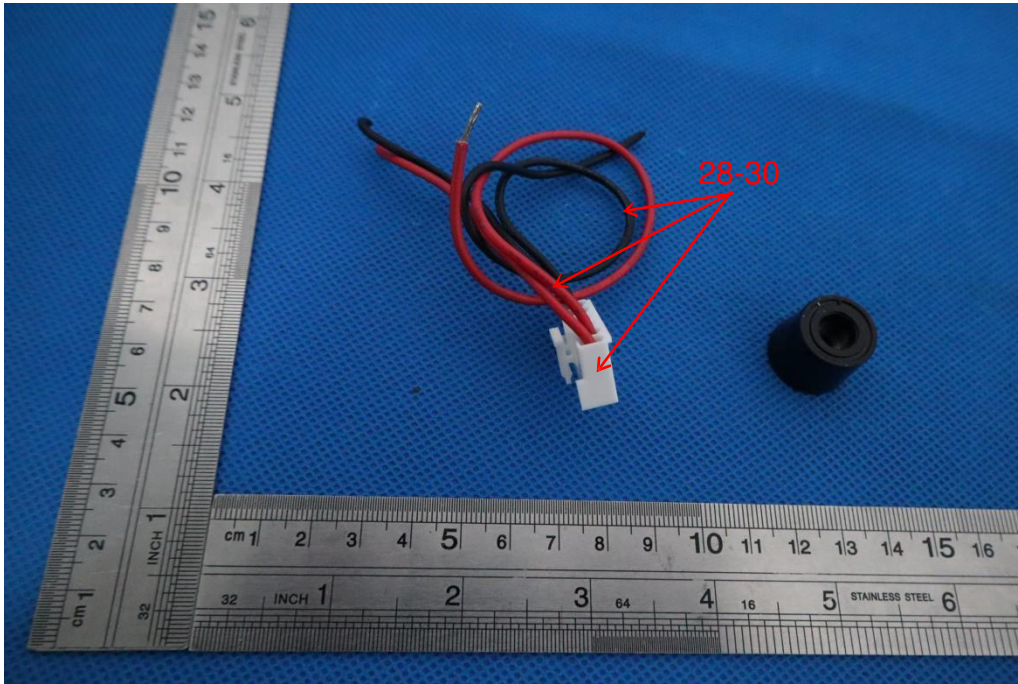


Fig.13

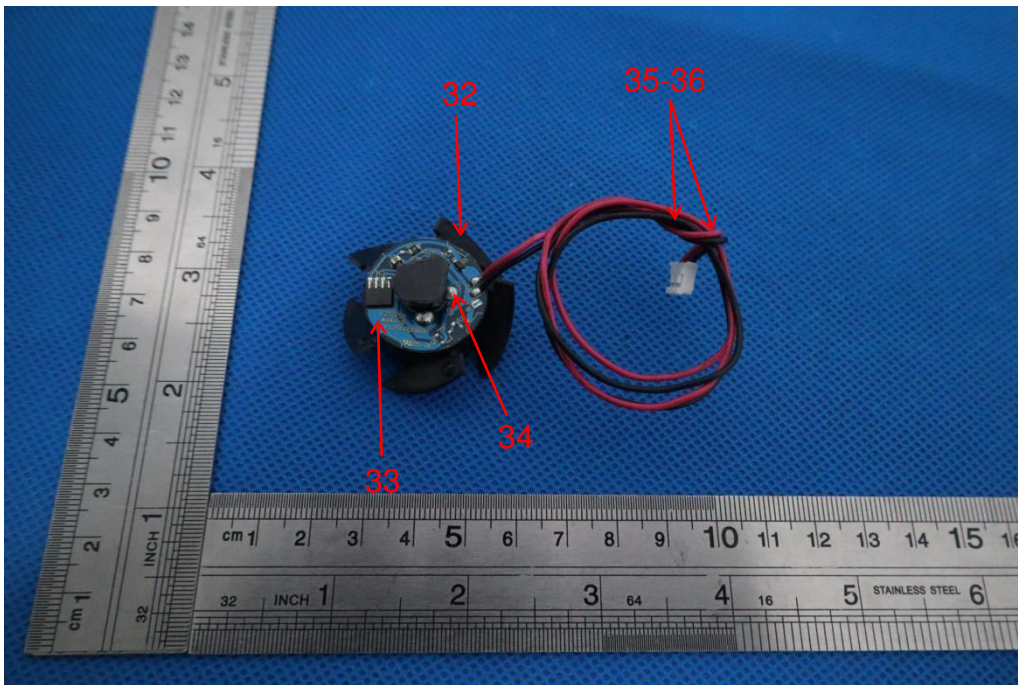
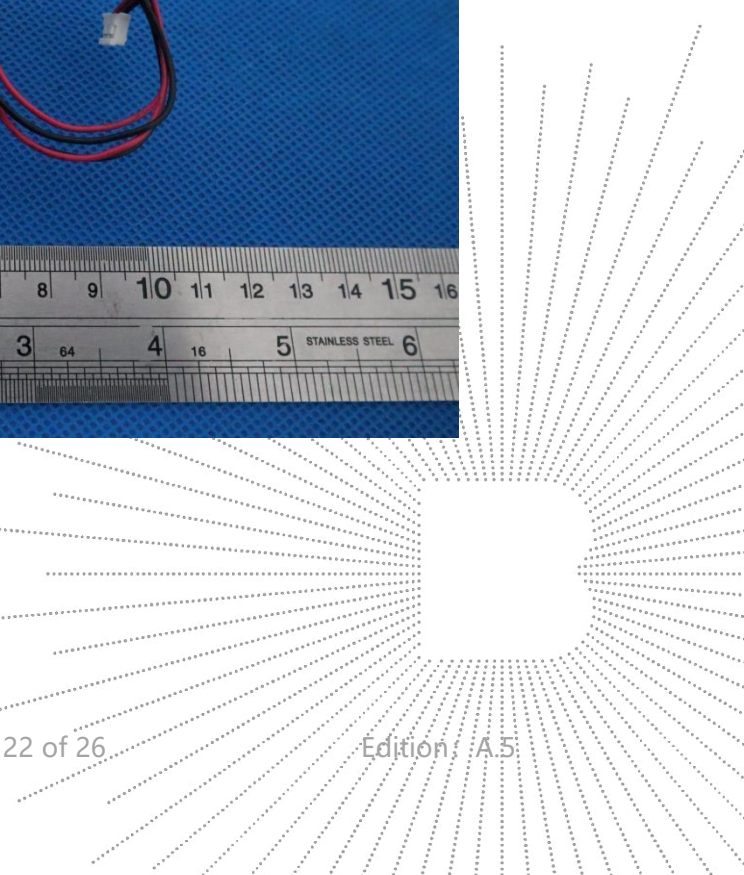


Fig.14

IC
C
PR
por



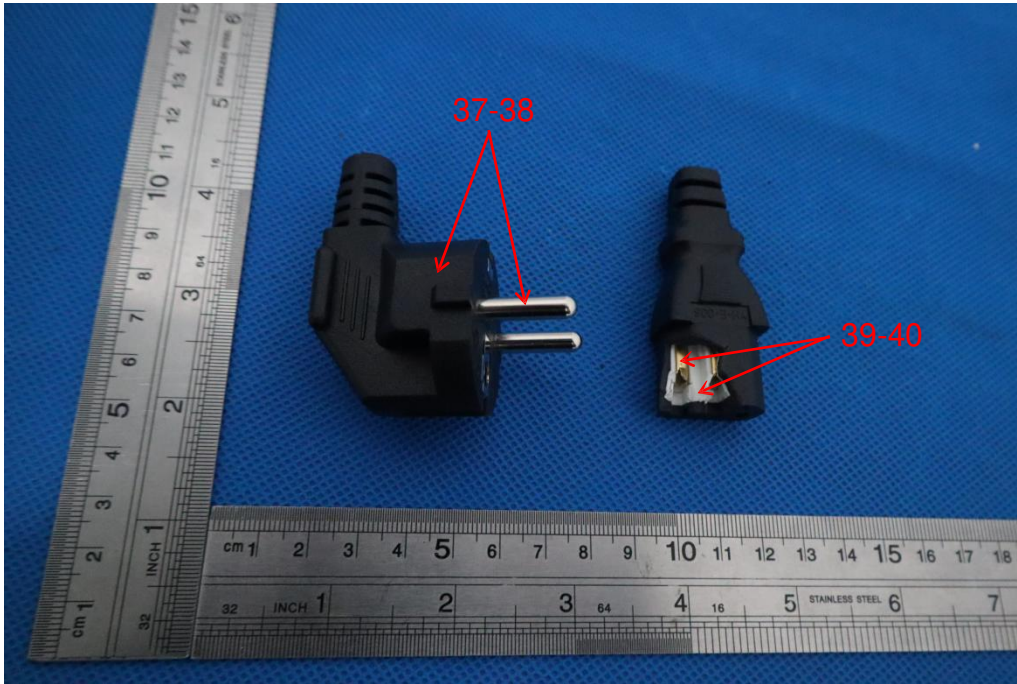


Fig.15

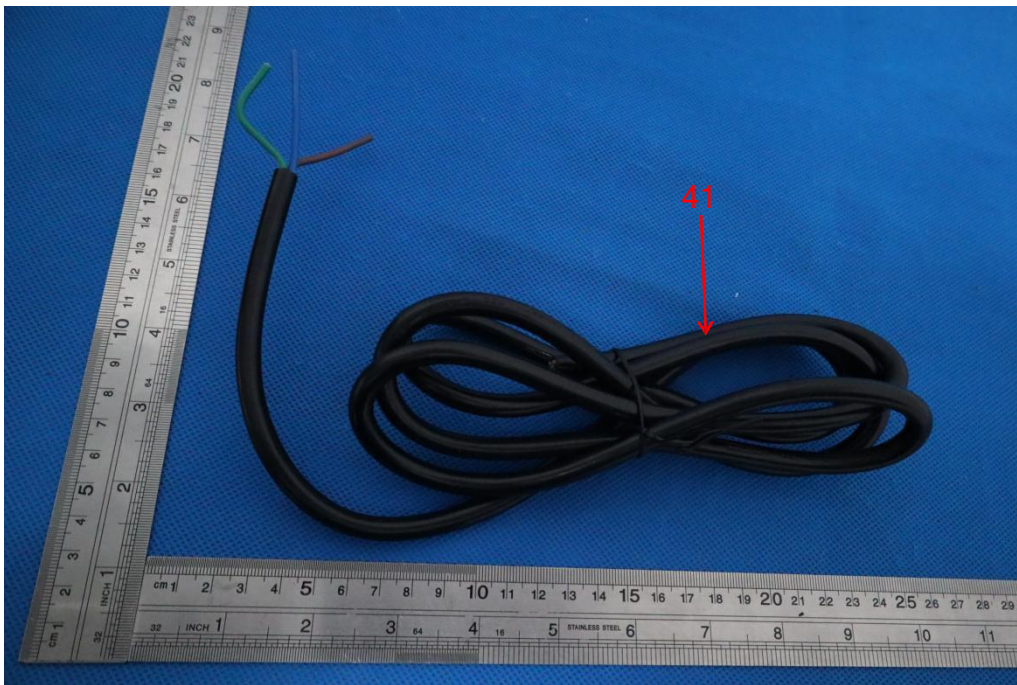
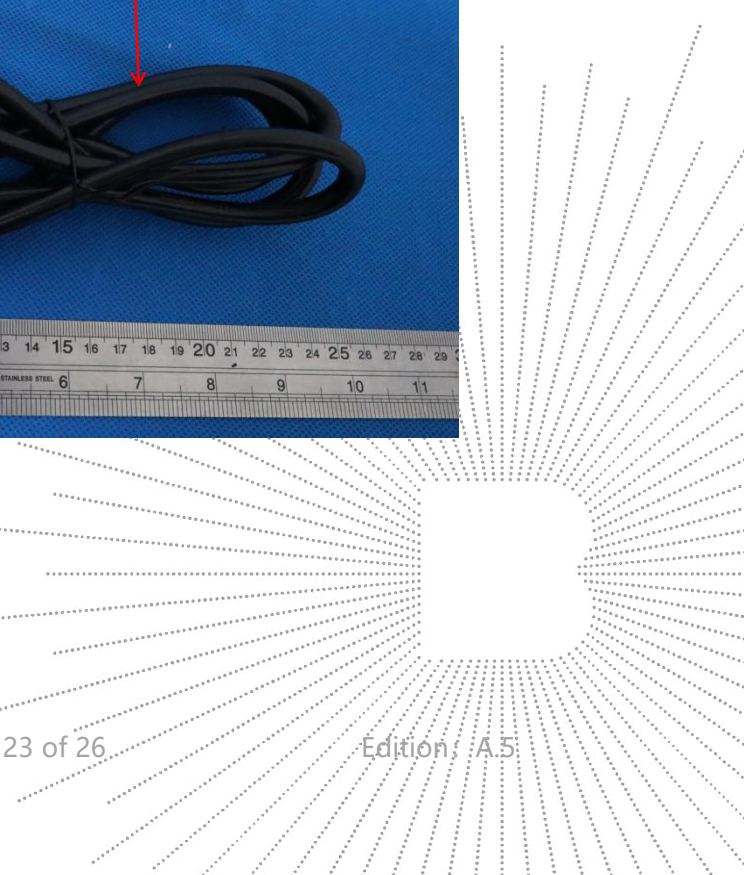


Fig.16

TE
T
OV
t Se



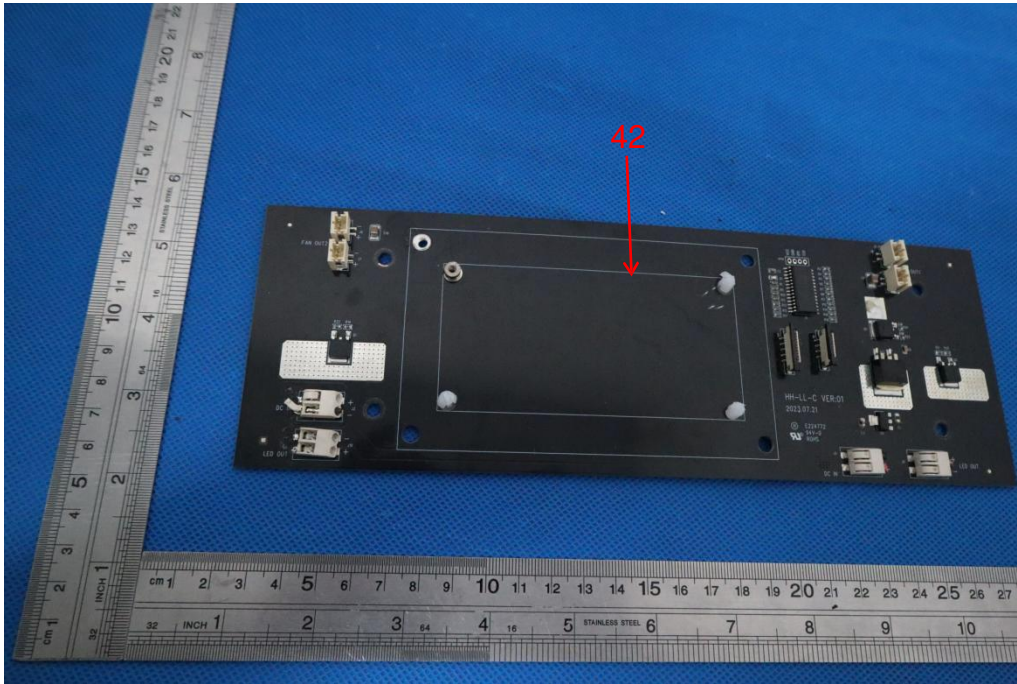


Fig.17

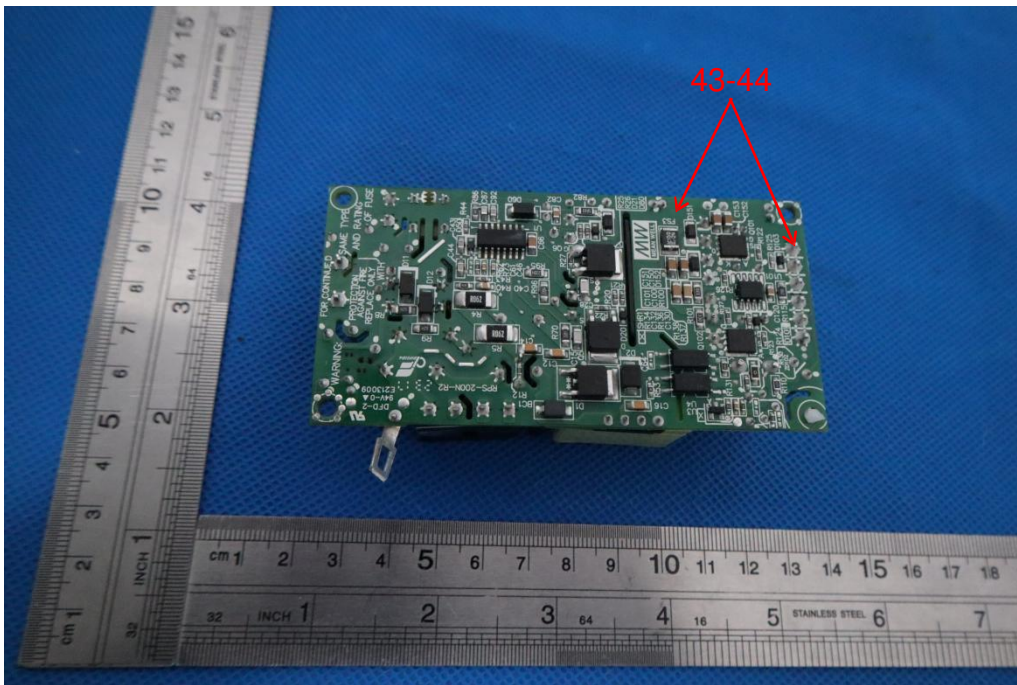
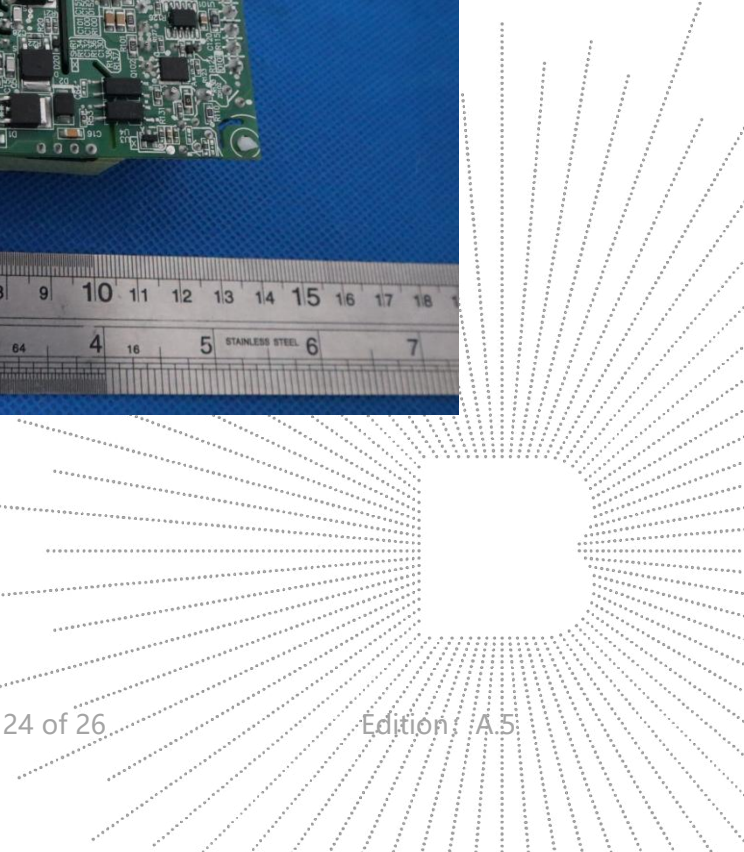


Fig.18

EST
C
ED
sal




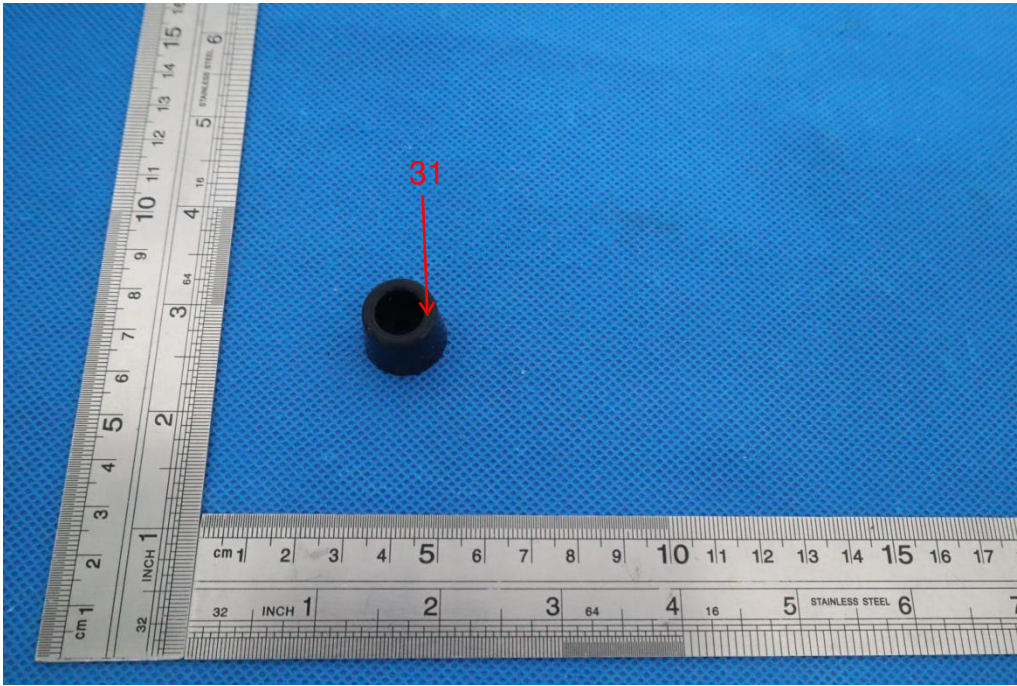


Fig.19

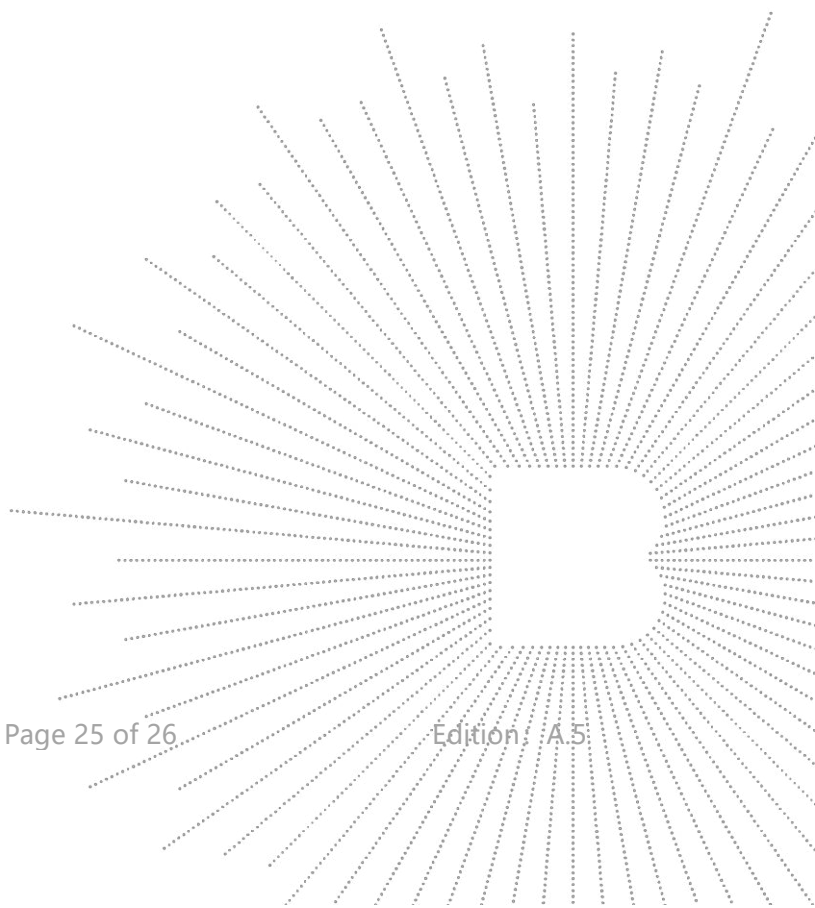

STATEMENT

1. The equipment lists are traceable to the national reference standards.
2. The test report can not be partially copied unless prior written approval is issued from our lab.
3. The test report is invalid without the "special seal for inspection and testing".
4. The test report is invalid without the signature of the approver.
5. The test process and test result is only related to the Unit Under Test.
6. Sample information is provided by the client and the laboratory is not responsible for its authenticity.
7. The quality system of our laboratory is in accordance with ISO/IEC17025.
8. If there is any objection to this test report, the client should inform issuing laboratory within 15 days from the date of receiving test report.

Address:

1-2/F., Building B, Pengzhou Industrial Park, No.158, Fuyuan 1st Road, Zhancheng, Fuhai Subdistrict, Bao'an District, Shenzhen, Guangdong, China

TEL: 400-788-9558

P. C. : 518103 FAX:

0755-33229357

Website: <http://www.chnbctc.com>

E-Mail: bctc@bctc-lab.com.cn

※※※※※ END ※※※※※

2017

